

# Dial Indicators

Comparison measuring instruments which ensure high quality, high accuracy and reliability.



An inspection certificate is supplied as standard. Refer to page X for details.

## SERIES 2 — Standard Type, 0.001mm & 0.005mm Graduation

- Standard 0.001mm and 0.005mm graduation dial indicators having a bezel with an outside diameter of  $\varnothing 57$ mm. All types come with limit markers and a bezel clamp.
- The outer clamp and lifting lever (optional) can be attached to either the right or left side. These parts can be easily installed and removed without tools.
- Secure adhesion between the bezel and crystal as well as the use of an O-ring prevents water or oil penetration.
- The spindle is made of high-strength quench-hardened stainless steel which resists arduous use.
- A carbide contact point is used.
- A special alloy is used for the sector gears to provide improved wear resistance.
- The indicator uses jeweled bearings, providing excellent indication sensitivity and durability.
- Application of a hard coating on the surface of the crystal makes the gauge highly scratch- and chemical-resistant.



21095-10



Balanced scale



Graduation: 0.001mm, Measuring range: 1mm

- 21095-10
- Shockproof type
- Jeweled bearing type



Continuous scale




Graduation: 0.001mm, Measuring range: 1mm

- 21105-10
- Double scale spacing type
- Shockproof type
- Jeweled bearing type



Balanced scale




Graduation: 0.001mm, Measuring range: 2mm

- 21135-10
- Shockproof type
- Jeweled bearing type



Continuous scale




Graduation: 0.001mm, Measuring range: 5mm

- 21185-10
- Jeweled bearing



Balanced scale




Graduation: 0.001mm, Measuring range: 5mm

- 21195-10
- Jeweled bearing




Continuous scale



Graduation: 0.005mm, Measuring range: 5mm

- 21245-10
- Jeweled bearing

## DIMENSIONS

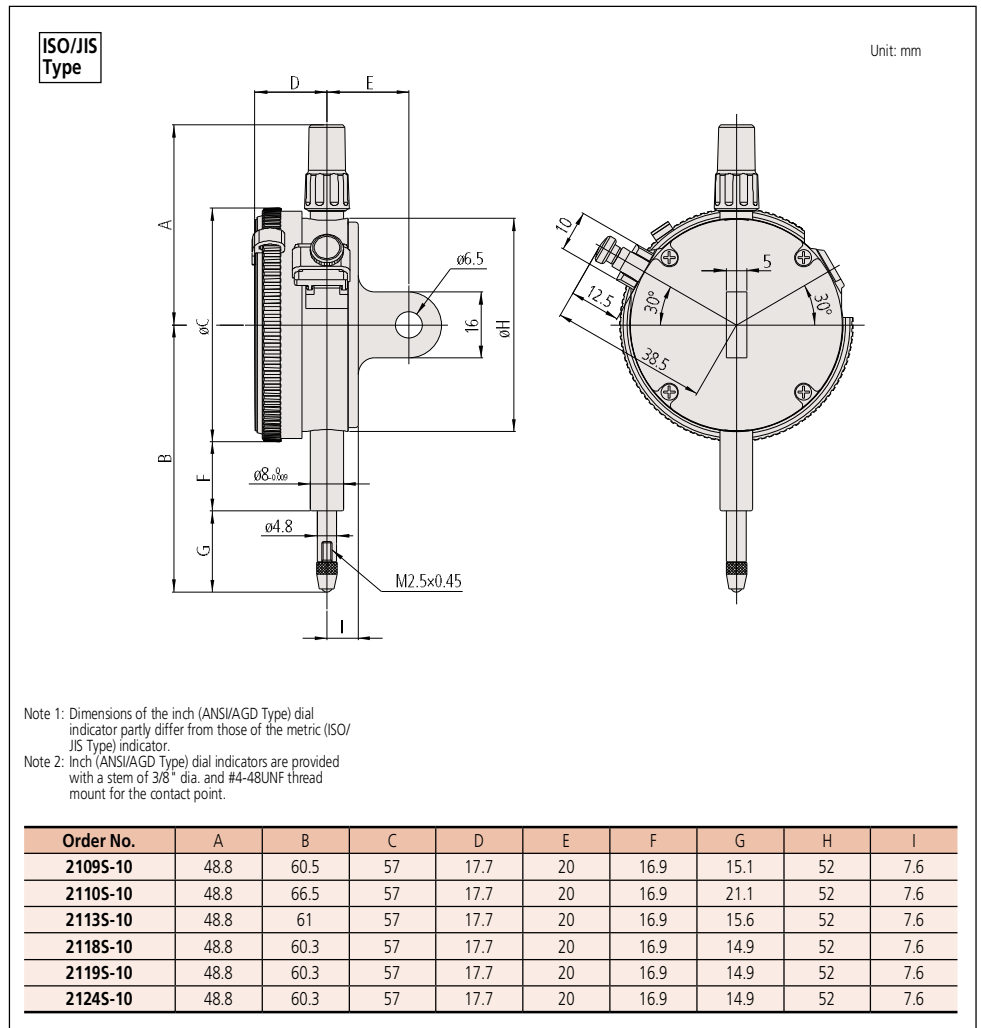

## FEATURES

Metric							
Order No.		1000	100	50	25	12.5	6.25
w/ lug	Flat-back	1000	100	50	25	12.5	6.25
2109S-10	2109SB-10	—	✓	✓	—	✓	—
2110S-10	2110SB-10	✓	—	✓	—	✓	✓
2113S-10	2113SB-10	—	✓	✓	—	✓	—
2118S-10	2118SB-10	✓	—	—	—	✓	—
2119S-10	2119SB-10	—	✓	—	—	✓	—
2124S-10	2124SB-10	✓	—	—	—	✓	—

## SPECIFICATIONS

Metric										ISO/JIS type
Order No.		Graduation	Range (range/rev)	Accuracy				Repeatability	Dial reading	Measuring force
w/ lug	Flat-back			Overall	Retrace	1/10 Rev	1 Rev			
2109S-10	2109SB-10	0.001mm	1mm (0.2mm)	5µm	2µm	2µm	4µm	0.5µm	0-100-0	1.5N or less
2110S-10	2110SB-10	0.001mm	1mm (0.1mm)	5µm	2µm	2µm	4µm	0.5µm	±0-100	1.8N or less
2113S-10	2113SB-10	0.001mm	2mm (0.2mm)	7µm	2µm	2µm	5µm	0.5µm	0-100-0	1.5N or less
2118S-10	2118SB-10	0.001mm	5mm (0.2mm)	10µm	3µm	3.5µm	6µm	1µm	0-100-100	1.5N or less
2119S-10	2119SB-10	0.001mm	5mm (0.2mm)	10µm	3µm	3.5µm	6µm	1µm	0-100-0	1.5N or less
2124S-10	2124SB-10	0.005mm	5mm (0.5mm)	12µm	3µm	5µm	9µm	3µm	±0-50	1.5N or less

\* Completed products inspection is performed in the vertical position (contact point downward) and the stated accuracy is guaranteed.