Compact Roundness Measurement ROUNDTEST RA-120/120P



Catalog No. E15008(2)

Compact roundness tester equipped with a wide range of analysis features and capable of flexibly accommodating a variety of workpieces




Roundtest RA-120



Simple, interactive display screen

The large LCD screen with backlight shows easy-to-understand measurement results and graphs. Forms can be checked and notch processing can be set while observing the displayed graphs.

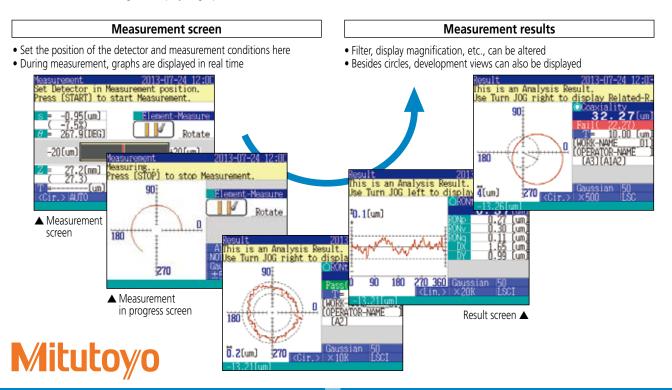

This compact roundness measuring machine is provided with numerous user-friendly features aimed at prioritizing usability, such as a wider range for the detector, an easy-to-understand operation panel with large LCD, a D.A.T. function that powerfully supports centering and leveling adjustments, and so on.

Operating panel that is read at a glance

Supports 16 languages

Japanese, English, German, French, Italian, Spanish, Portuguese, Korean, Traditional Chinese, Simplified Chinese, Czech, Polish, Hungarian Turkish, Swedish, Dutch

Analysis type

Selection buttons provide access to a wide variety of analysis types

Switching screen modes

Switch the display at the touch of a button, providing access to the [Calibration], [Centering and Leveling], [Measurement], and [Result] screens.

Zero-setting button

No fine adjustment necessary for setting the measurement position



Simple setup

Apply the current measurement setup in one go Simple operation helps prevent operational errors

Jog dial


Make detailed changes to setup and other operations

Simplified communication program for ROUNDTEST RA-120

The Roundtest RA-120 has a USB interface, enabling data to be transferred to a spreadsheet or other software.

Notch processing


Unwanted data, such as that produced by notches or scratches, can be excluded from the analysis if desired. Select between [Automatic setting] and [Arbitrary setting].



High-grade thermal printer

Print measurement conditions, computation results, result graphs, comments, etc., to the thermal printer. Change development graphs and output items as desired.

■ Sample prints




Recording paper set (optional set of 10 rolls)

File save

Save and access [Measurement files] and [Result files] in USB memory. Data can also be totaled using the data output function with commercial tabulation software.


[Measurement file] [Measurement data (Data output)] [Result file] [Result data (Data output)]

Roundtest RA-120P

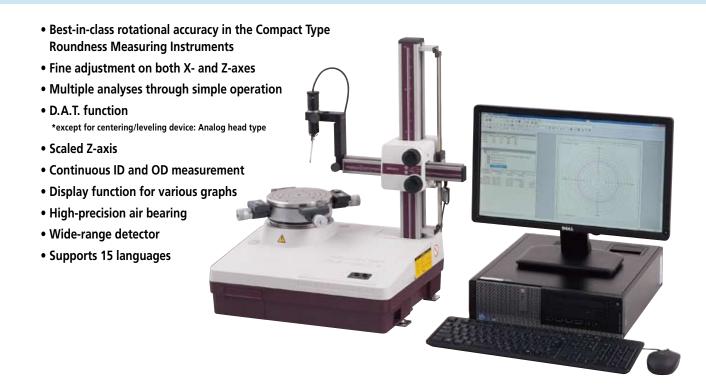


Windows graphical interface

By using a mouse and buttons, identified by corresponding icons, to control the machine, the Roundtest RA-120P's interface provides excellent usability. Functions such as recalculation and graph reading are handled swiftly with easy-to-understand operations.

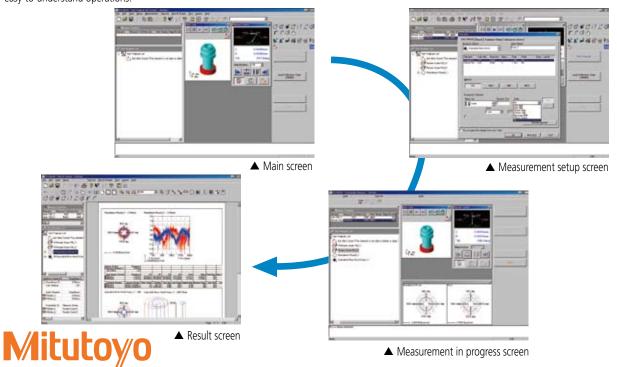


This entry-level desktop tester incorporates the ROUNDPAK multi-analysis evaluation program, which provides it with analytical power close to that of more elaborate models. This is, therefore, a highly functional multi-analysis roundness measuring machine that is suitable for use not only in measurement rooms, but also in research and development sections.


Measurement screen makes ample use of graphs

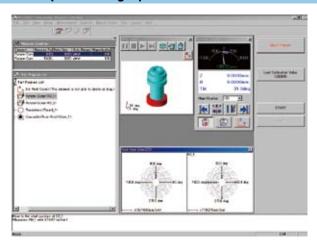

Multi-analysis function


Complete with a wide range of functions including partial enlargement, auxiliary line setup, color change, displacement/angular difference of data between two points, and so on. Also equipped with notch processing and graph reading functions, which make the machine useful in research departments. Recalculation can also be performed with the filter and evaluation method changed.






Simplified layout function


Computation results for multiple items can be laid out in multiple forms on a single sheet and printed. This function also supports output to a color printer (optional).



■ Layout setting screen



■ Sample print outputs



Functions that implement greater efficiency of measurement and range of analysis types


D.A.T. function *except for centering/leveling device (analog micrometer heads)

This instrument uses the D.A.T. (Digital Adjustment Table) function available on more sophisticated models, and this provides powerful support for centering and leveling operations. To perform such operations, the user need only adjust the digital micrometer heads attached to the rotary table by the amounts indicated by the display. This function also supports measurement of notched workpieces.






RA-120










RA-120P

















Displays amount of offset/inclination





Centering/leveling complete

Continuous ID and OD measuring function

This function comes in very handy when outside diameter and inside diameter surfaces need to be measured repeatedly, for example, with respect to coaxiality, deviation in wall thickness, etc. The inner surface can be measured and evaluated with the detector, maintaining the same measuring position for the outside diameter without changing its orientation, as illustrated on the right.

Inside diameters down to 50mm can be measured.



Continuous inside and outside diameter function (inside dia. surface)



Continuous inside and outside diameter function (outside dia. surface)

Z-axis scale


This scale is useful when the measuring height position needs to be entered, such as when measuring coaxiality, etc. The machine uses an ABS Digimatic scale unit to provide an effective means for repetitive measurement and position setting.





IN/OUT switchable wide-range detector

The range of this detector has been extended from that of a conventional lever head by as much as four times, and is now wider than ever before. The detector can provide sufficient margin for centering and leveling jobs, or when measuring large differences. Moreover, the measuring direction can be switched between inside and outside diameters with a single touch of a button.

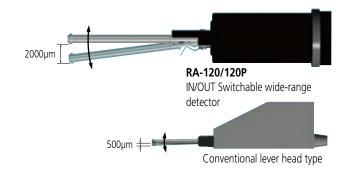


Types of Analysis

Typ Ana	e of lysis	Measurement möde	Evaluation diagram	RA- 120	RA- 120P
2000	Scalinies S			0	0
1004	rianiess		Against Akis 8	0	0
eness	Relative to Axis	40	Axis Sg	0	0
Squareness	Relative to Plane Relative to Axis		batum plane	0	0
74:0:34	Concentration		2xC	0	0
Coaxality	Of section	Axis 2 N	žxc	0	0
Coa	Of axis	Axis 1		_	0

Type of Analysis		Measurement	Evaluation diagram	RA- 120	RA- 120P
Parallelism				0	0
Thickness variation Axial Radial		4	12-11	0	0
		4	(2) r1	0	0
Circular run-out	Radial	N ر		0	0
Circular	Axial			0	0
Power spectrum				_	0
Profile	Profile operation		= +++++++++++++++++++++++++++++++++++++	_	0

Optional Accessories

■ Interchangeable Styli

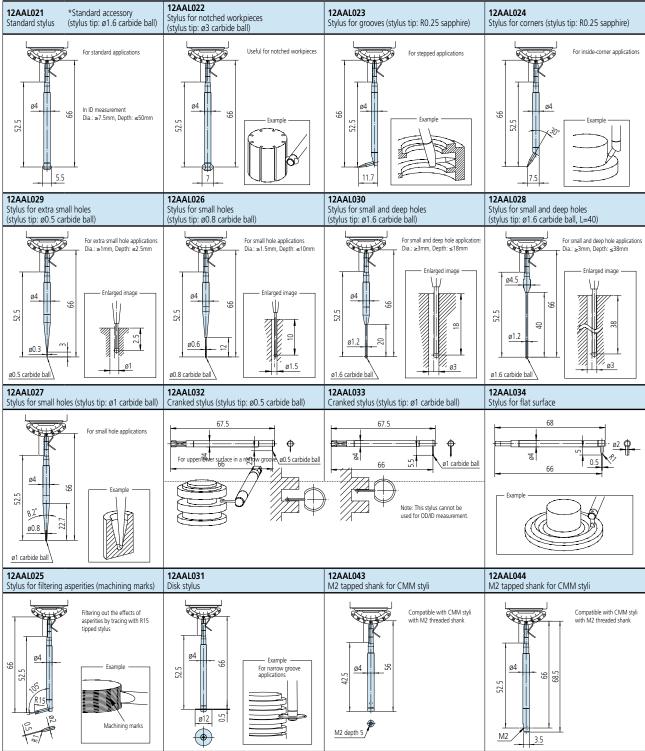



^{*} portion shows stylus except for the cranked stylus and stylus for flat surface.

*() dimension shows a distance from the tip end of stylus or the center of tip ball to the connecting surface of detector.

*Customized special interchangeable styli are available on request. Please contact any Mitutoyo office for more information.

Centering chuck (knurled ring operated)

Provides good operability when measuring a small-diameter workpiece. The knurled ring allows the workpiece to be clamped easily.



Order No.	211-032
Holding range	OD with internal jaws 1–36 mm ID with internal jaws 16–69 mm OD with internal jaws 25–79 mm
External size (D x H)	
Mass	1.2 kg

Collet chuck

Provides high clamping repeatability due to the use of optional precision collets. (See table at right.)



Order No.	211-051
Part holding range	ø0.5–10 mm* ²
Centering error	Within 50 µm* ³
Mass	1.4 kg

^{*2:} Collets to match the workpiece size range are required for use with this chuck.

*3: When measured with ø5 mm pin gauge at measuring height of 30

X-axis stop

Allows the user to return the detector rapidly and easily to a fixed position in the X axis.



Order No.	12AAH320
Mass	65 a

■ Three-jaw chuck (key operated)

Useful where it is necessary to apply a higher clamping force to the workpiece than can be applied with the centering chuck.



Order No.	211-014
Holding range	OD with internal jaws 2–26 mm ID with internal jaws 25–68 mm OD with internal jaws 35–78 mm
External size (D x H)	
Mass	3.8 kg

■ Individual collets*4

These collets are for use with the collet chuck shown at left and are acquired to match the workpiece diameter range required.

Part Holding Range
ø0.5–1.0 mm
ø1.0–1.5 mm
ø1.5–2.0 mm
ø2.0–2.5 mm
ø2.5–3.0 mm
ø3.0–3.5 mm
ø3.5–4.0 mm
ø4.0–5.0 mm
ø5.0–6.0 mm
ø6.0–7.0 mm
ø7.0–8.0 mm
ø8.0–9.0 mm
ø9.0–10.0 mm

^{*4.} A collet cannot be mounted on the rotary table without a collet chuck. *4: YCC10-** Class AA, made by Yukiwa Seiko Inc. or its equivalent.

■ Vibration-damping stand



Order No.	211-013		
Vibration damping system	Diaphragm type air spring		
External size	615 x 515 x 51 mm		
Max. loading mass	150 kg		

■ Microchuck

For clamping a small workpiece, 1 mm or less in diameter, that cannot be held in the centering chuck.



Order No.	211-031
Holding range	OD: up to 1.5 mm
External size (DxH)	ø118 x 48.5 mm
Mass	0.6 kg

■Auxiliary stage for a short workpiece

Order No. 356038



■ Reference hemisphere

Order No. 211-016



■ Magnification checking gage

Order No. 211-045



■ Gage block set for calibration

Order No. 997090



Replacement elements for the air filter


Order No. 358592 (for filter) 358593 (filter regulator)

■ Simplified communication program for ROUNDTEST RA-120

The Roundtest RA-120 has a USB interface, enabling data to be transferred to a spreadsheet or other software. We also provide a program that lets you create inspection record tables using a Microsoft Excel* macro.







Required environment:

- OS: Windows XP-SP3 Windows 7
- Spreadsheet software: Microsoft Excel 2010
- *Windows OS and Microsoft Excel are products of Microsoft Corporation.

The optional USB cable is also required.

• USB cable for **RA-120** series Order No. 12AAH490


Specifications

■ Main unit


Madal		RA-120			RA-120P			
Model		Dedicated electronic analysis type			Data analysis by PC			
	Rotational Radial		(0.04+6H/1	0000)µm H: Probi	ng height (mm) JISB	7451-1997		
	accuracy Axial	(0.04+6X/10000)µm X: Probing radius (mm)						
	Rotational speed	6rpm						
	Effective table diameter	150mm						
	Centering range adjustment		±3mm					
Turntable	Leveling range adjustment			±	1°			
	Centering/leveling device (micrometer head)	Analog head	Digital head (mm)	Digital head (inch/mm)	Analog head	Digital head (mm)	Digital head (inch/mm)	
	Maximum probing diameter		280mm (3	880mm in a reverse	e and vertical detector position)			
	Maximum workpiece diameter			440	mm			
	Maximum turntable loading			25	kg			
	Vertical travel			280mm from th	ne turntable top			
Vertical column (Z axis)	Maximum probing height	280n	nm from the turntab	le top (480mm in th	e reverse and vertic	al detector configu	ration)	
	Maximum probing depth			100mm (minim	ium ID: 30mm)			
Horizontal arm (X axis)	Horizontal travel		165mm (Including	a protrusion of 25n	nm from the turntal	ole rotation center)		
	Measuring direction			Two directional (IN	I/OUT switchable)			
D. I I	Measuring range			±100	10μm			
Detector	Measuring force			70 to 100mN (±30%)				
	Standard stylus (12AAL021)	Carbide ball, Ø1.6mm (.06")						
	Measuring range	8 steps: ±(1000, 500, 200, 100, 50, 20, 10, 5)µm						
	Magnification		X5 to X200,000			X1 to X500,000		
	Filter type	Phase corrected: Gaussian, 2CRPC75, 2CRPC50 Not phase corrected: 2CR75, 2CR50 Filt				Filter OFF		
	Cutoff value		or, 50upr, 150upr, 50 Jupr, 15-500upr, 50-)upr, 150upr, 500up 15-500upr, 50-500		
	Number of measuring sections		Maximum 5			Maximum 100		
	Evaluation type	Roundness, coaxality, concentricity, flatness, circular run-out (radial/axial), squareness (relative to axis/plane), thickness deviation, parallelism						
	Reference circle for evaluation	LSCI, MZCI, MICI, MCCI						
Electronic unit	Adjusting centering/leveling	DAT function (circular/multi-point switchable)						
	Functions	Notched measurement, re-calculation, limaçon error correction, continous ID and OD measurement Notched measurement, correction, remarkable panalysis, continous I			rkable point analysis	s (gear), harmonic		
	Printer	Thermal line	printer, optional ex	ernal printer	Windov	vs compatible ink-je	et printer	
	Display languages	Japanese, English, German, French, Italian, Spanish, Portuguese, Korean, Traditional Chinese, Czech, Polish, Hungarian Turkish, Swedish, Dutch Japanese, English, German, French, Italian, Spanish, Portuguese, Korean, Traditional Chinese, Czech, Polish, Hungarian		rean, Traditional Ch	inese, Simplified			
	USB stick memory	Calculation result, measurement data						
	Data output RS-232C	Calculation result, measurement data						
	SPC	Calculati			tion result			
	Power supply	AC 100) – 240V			
	Power consumption	32 – 36W 21 – 24W (excluding PC system)					system)	
Others	Air pressure		0.39MPa					
	Air consumption	30L/min (minimum)						
	Mass	Main unit: 32kg Air filter: 2kg						




Dimensions

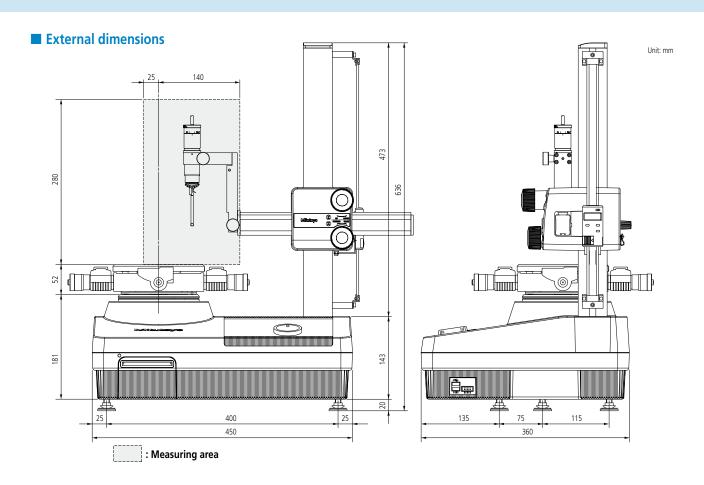


■ Turntable top view

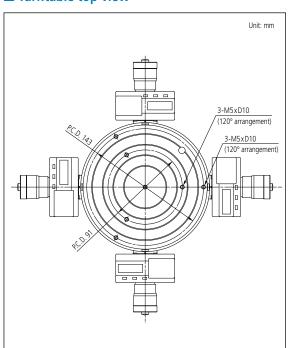

■ Installation floor plan

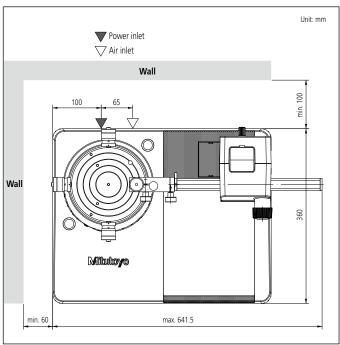

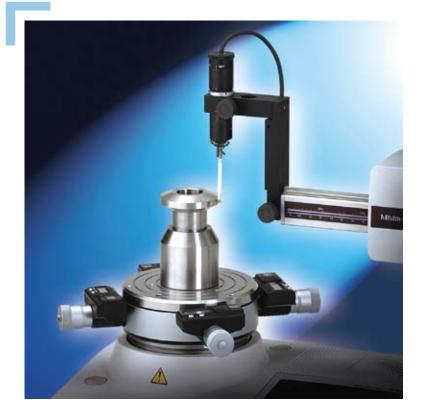

Specifications are subject to change without notice.

Export permission by the Japanese government may be required for exporting our products according to the Foreign Exchange and Foreign Trade Law. Please consult our sales office near you before you export our products or you offer technical information to a nonresident.

Coordinate Measuring Machines

Vision Measuring Systems

Form Measurement

Optical Measuring

Sensor Systems

Test Equipment and

Digital Scale and DRO Systems

Small Tool Instruments and Data Management

Mitutoyo Corporation

20-1, Sakado 1-Chome, Takatsu-ku, Kawasaki-shi, Kanagawa 213-8533, Japan T +81 (0) 44 813-8230 F +81 (0) 44 813-8231 http://www.mitutoyo.co.jp

Note: All information regarding our products, and in particular the illustrations, drawings, dimensional and performance data contained in this pamphlet, as well as other technical data are to be regarded as approximate average values. We therefore reserve the right to make changes to the corresponding designs, dimensions and weights. The stated standards, similar technical regulations, descriptions and illustrations of the products were valid at the time of printing. Only quotations submitted by ourselves may be regarded as definitive.

